




## DESCRIPTION AND INTENDED USE

**MINI MITO BTE PRO POWER:** Mini Mito, miniBTE digital hearing aid, battery 312. It is intended to compensate for mild to severe hearing losses. Easy to wear and comfortable. Powerful receiver for a better performance. Six (6) channels WDRC hearing aid, 12 adjusting bands (equalizers), 4 memories, feedback notch filter, low and high cut filters, output limiting. Moreover, Adaptive feedback cancelling and Noise reduction and Adaptive directional microphone processing available.

## FEATURES

- 6-Channel Wide Dynamic Range Compression (WDRC) with Dynamic Contrast Detection™
- Patented Adaptive Feedback Cancelling
- Layered Noise Reduction™
- Two Compression Adjustment Paradigms
- Adaptive Directional Microphone Processing
- Program Selector
- Battery Type: 312

## FITTING RANGE

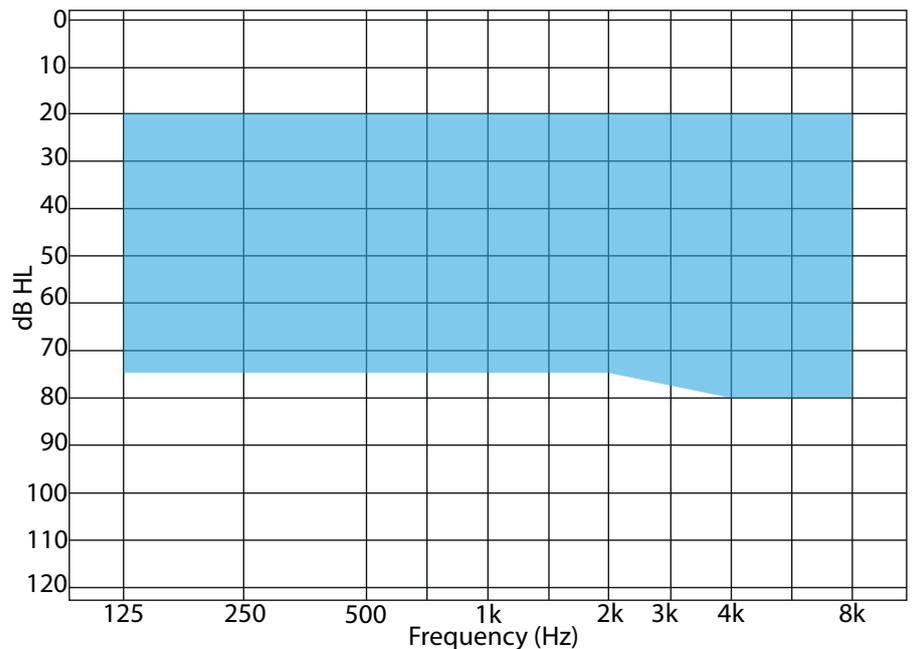

**WARNING!**  
 This hearing aid can generate sound output levels in excess of 132 dB<sub>CP</sub> (IEC 60318-4 Coupler).  
 The hearing care specialist should be specially careful fitting the instrument as there may be risk of impairing the remaining hearing of the hearing instrument user.

**CE** FDA Approved  
 1370

<b>Technical data</b> <i>Measured according to</i>		<b>EAR SIMULATOR</b> <i>IEC 60118-0:2015 and IEC 60318-5:2006</i>	<b>2CC Coupler</b> <i>ANSI S3.22-2014, IEC60118-7:2005 and IEC 60318-5:2006</i>
<b>Horentek Mini Mito</b>		<b>PRO POWER</b>	<b>PRO POWER</b>
Frequency range Hz		200/5500 Hz	200/5500 Hz
OSPL90	Peak Measurement	-	-
	Peak 1400 Hz	131 dB	126 dB
	HFA AVERAGE	123 dB	118 dB
Full-on gain 50*	Peak Measurement	-	-
	Peak 1400 Hz	76 dB	71 dB
	HFA AVERAGE	54 dB	51 dB
Reference test gain		46 dB	41 dB
Telecoil output (1600 Hz)	1 mA/m field 10 mA/m field SPLITS L/R	-	-
Total harmonic distortion (input 70 dB SPL)	500 Hz	< 2 %	< 2 %
	800 Hz	< 2 %	< 2 %
	1600 Hz	< 2 %	< 2 %
Equivalent input noise level		49 dB SPL	49 dB SPL
Battery consumption**(Battery 312) Typical		0.54 mA	0.54 mA
Battery life, artificial measurements, hours ***		305	305



\* Measured with the gain control of the hearing aid set to its full-on position minus 20dB and with an input SPL of 70 dB.  
 \*\* Battery current is measured according to IEC 60118-0:2015 §7.7 after a settling time of a minimum of 3 minutes  
 \*\*\* Based on the standardized battery consumption measurement. The actual battery life depends on battery quality, use pattern, active feature set, hearing loss and sound environment.

Data may vary by more or less 5%



Ear simulator

2CC Coupler

OSPL90

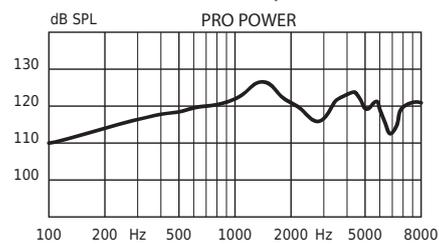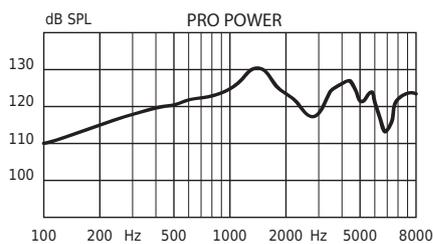

Full-on Gain

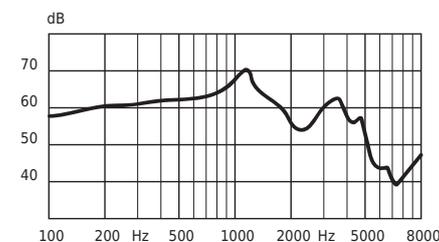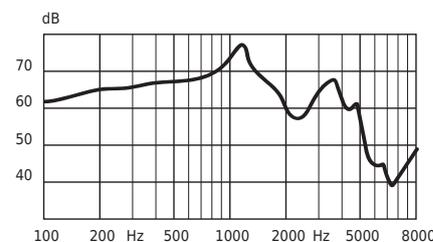

Frequency Response

